

We are IntechOpen, the world's leading publisher of Open Access books Built by scientists, for scientists

6,900

Open access books available

186,000

International authors and editors

200M

Downloads

Our authors are among the

154

Countries delivered to

TOP 1%

most cited scientists

12.2%

Contributors from top 500 universities



WEB OF SCIENCE™

Selection of our books indexed in the Book Citation Index
in Web of Science™ Core Collection (BKCI)

Interested in publishing with us?
Contact book.department@intechopen.com

Numbers displayed above are based on latest data collected.
For more information visit www.intechopen.com



Electrochemical Biosensors for Virus Detection

Adnane Abdelghani

*National Institute of Applied Science and Technology, Charguia Cedex
Tunisia*

1. Introduction

The rabies constitutes one of the most dangerous viruses causing many death cases every year. Each year approximately 55,000 people die of rabies, with high percentage of children [S et al., 2007; L et al., 2000; FX et al., 1994]. High percentages (99%) of the registered cases were in Asia and Africa. In order to fight this dangerous disease, many techniques are usually used for diagnostic but are usually complex, time consuming, expensive, difficult to implement, and this is a necessity for developing new detection process [N et al., 1993; Crepin et al., 1998]. Avian Influenza Virus (AIV) infections are a major cause of mortality and rapid identification of the virus has important clinical, economical and epidemiological implications. The traditional methods for virus diagnostic are Enzyme Linked Immunosorbent Assay (ELISA) and Reverse Transcriptase Polymerase Chain Reaction (RT-PCR) which are time consuming and expensive. Biosensors can play an important role in areas such as diagnostic of diseases, drug detection and food quality control. Biosensors are devices with qualities quoted as rapidity, sensitivity and specificity [G et al., 2002; D et al., 1999]. Biacore based on Surface Plasmon Resonance technique is effectively a successful biosensor used for antigen-antibody interaction [J et al., 1999]. Others commercialized biosensors such as glucometer was developed for self-monitoring of glucose in blood for diabetes care.

In terms of the transduction techniques used, the three main classes of biosensors are optical, electrochemical and piezoelectric. Out of the three, optical methods appear to be the most sensitive, with surface plasmon resonance and waveguide based devices being the technological spearhead. As for Electrochemical biosensors, they are cheaper than optical ones. They can be amperometric or impedimetric, depending on whether they monitor a current as a function of potential or the resulting sensor impedance as a function of frequency. The advantage of impedimetric methods is that, unlike amperometry, they do not need of enzymatic labels in order to detect. In this work, we use the high sensitive impedance spectroscopy technique for biosensors applications. This technique is very known to characterize the electrical properties of materials and their interfaces exposed to electronically conducting electrodes [A et al., 2004; S et al., 2006; A et al., 2006]. It may be used to investigate the dynamics of bound and mobile charges in the bulk or interfacial regions of any kind of solid or liquid material: ionic semiconducting, mixed electronic-ionic and dielectric. The biosensor is based on the immobilization of specific anti-rabies polyclonal antibodies and specific anti-H₇N₁ antibodies onto a functionalized gold electrode with micrometer size. The affinity interaction of the antibody with the specific antigen can

be measured with a good reproductibility with impedance spectroscopy [M et al., 2008; M et al., 2008]. The different steps of biosensor conception were characterized by Electrochemical Impedance Spectroscopy (EIS). The obtained limit detection was better than those obtained with the others traditional methods for clinical use. The non-specific interaction has been tested with the Newcastle antigen virus.

2. Experimental set-up

2.1 Specific rabies antibody preparation

Rabies immunoglobulins were produced by horse immunization. The immunization was carried out using human vaccine "RABIPUR" manufactured by "Chiron Behring Vaccines" in Ankleshwar (Gujarat), India. The horses were exposed to a series of injections to increase vaccine amounts. The immunization period lasted for 105 days (M et al., 2008).

2.2 Specific rabbit antibody (anti-H₇N₁) preparation

Three male rabbits were injected sub-cutaneously with different doses of NobilisTM, INFLUENZA H₇N₁ vaccine in different periods (15 days, 30 days, 45 days, 65 days). For each period, quantity of blood were analysed to study the kinetic of the rabbit vaccine immuno-response. Hyper immuno serums has been collected and specific rabbit-polyclonal antibodies (anti-H₇N₁) has been purified with affinity chromatography (M et al., 2008).

2.3 Antibody immobilization on gold electrode

The gold electrodes were cleaned with organic solvents (acetone and ethanol) and with piranha solution (1:3 H₂O₂ - concentrated H₂SO₄) for 1 min. After each treatment, the gold substrates were rinsed with ethanol and dried under nitrogen flow. The pretreated electrodes were immersed in 11-mercaptopundecanoic acid 1 mM in ethanol solution for 12 h in order to form a self-assembled monolayer (SAM). The substrates were then rinsed with ethanol in order to remove the unbonded thiols. To convert the terminal carboxylic groups to an active NHS ester, the thiol-modified electrodes were treated with 0.4 mM EDC-0.1 mM NHS for 1 h. After gold electrodes were rinsed with water and dried under nitrogen, 20 µg/ml of Anti-Rabies IgG (respectively 5 µg/ml of Anti-H₇N₁) were dropped onto the surface at 37 °C for one hour. The excess antibodies were removed by rinsing with PBS. Then, the antibody-modified electrodes were treated with 0.1% BSA for 30 min, to block the unreacted and non-specific sites. After rinsing with PBS and water, the electrodes were dried under nitrogen (Figure.1).

2.4 Impedance spectroscopy

Many reports show that impedance spectroscopy is a useful tool to characterize self assembled monolayer on surfaces (A et al., 2004). A capacitor is formed between the conducting electrode and the electrolyte. The absolute impedance is related to the frequency by the equation:

$$|Z| = \frac{1}{2\pi fC} \quad (1)$$

where f is the frequency (in Hz) at which Z is measured.

The complex impedance can be presented as a combination of the real impedance (Z_{re}) and imaginary impedance (Z_{im}), Nyquist plot. To fit the measured spectra with the impedance spectra out of ideal elements, the ideal elements have been replaced with the constant phase elements (CPE):

$$Z_{CPE} = K\omega^{-\alpha} \quad (2)$$

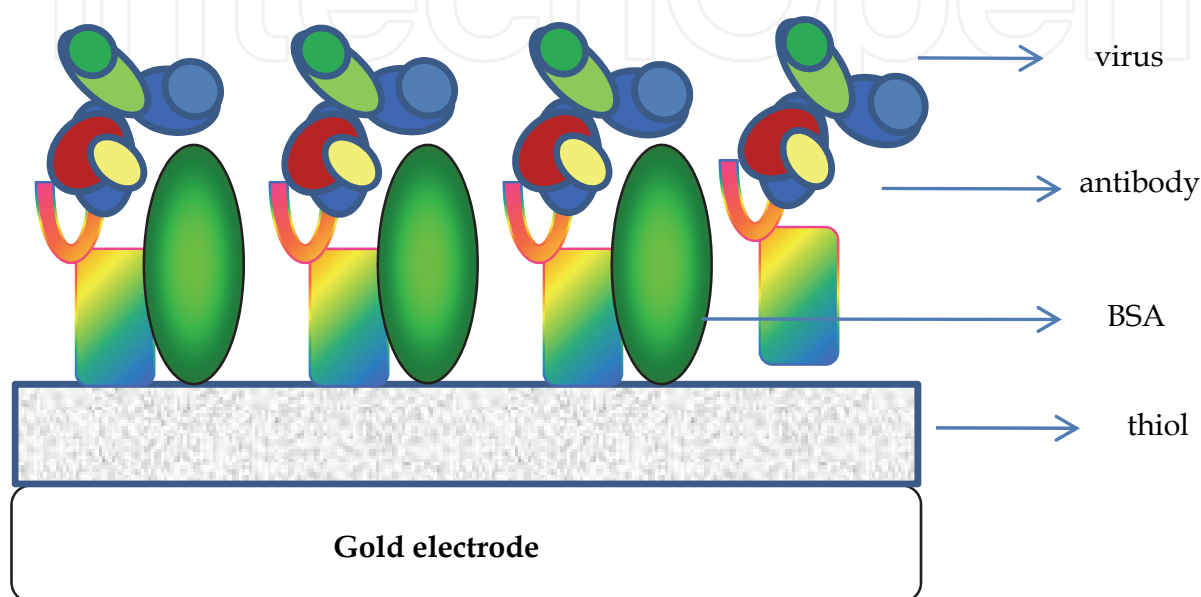


Fig. 1. Biosensor multilayer configuration

The frequency exponent is $\alpha = 1$ and $K = 1/C$ for an ideal capacitance, and $\alpha = 0$ and $K = R$ for an ideal resistance, respectively. The exponent α could be obtained, when the membrane capacitance (or layer capacitance) was replaced by a constant phase element Z_{CPE} . The deviation of the exponent α from the ideal values is attributed to the inhomogeneities of the analyzed layer, like defects or roughness. The measured spectra of the impedance were analyzed in terms of electrical equivalent circuits using a analysis program. The mathematical expressions of the equivalent circuit models were fitted to the data. The electric parameters of the system were calculated with the computer program and the fit error was kept under a maximum of 10%. The impedance analysis was performed with the Voltalab 40 impedance analyser in the frequency range 0.05 Hz - 100 kHz, using a modulation voltage of 10 mV. Three-electrode system was employed with a saturated calomel electrode (SCE), an immunosensor working electrode (0.19 cm²), and a platinum strip counter electrode (0.385 cm²). The impedance measurements were performed in the presence of a 5 mM $K_3[Fe(CN)_6]/K_4[Fe(CN)_6]$ (1:1) mixture as redox probe in PBS. The measured spectra of the impedance and phase were analysed in terms of electrical equivalent circuit model using a Zview modelling programme (Scribner and associates, Charlottesville, VA). All electrochemical measurements were carried out at room temperature and in a faraday cage. More details on electrochemical impedance spectroscopy can be found in reference (A et al., 2004; M et al., 2008).

3. Results and discussions

3.1 Avian influenza virus biosensor

First, we study the variation of the impedance spectra (the real part, it means the charge transfer resistance) of the functionalized gold electrode with different concentration of immobilised antibody. This allows us to know the saturation concentration of the antibody on our gold electrode, which will leads to the high sensitivity detection. Figure.2 shows the impedance spectra of the functionalized gold electrode after the immobilisation of antibody with different concentration.

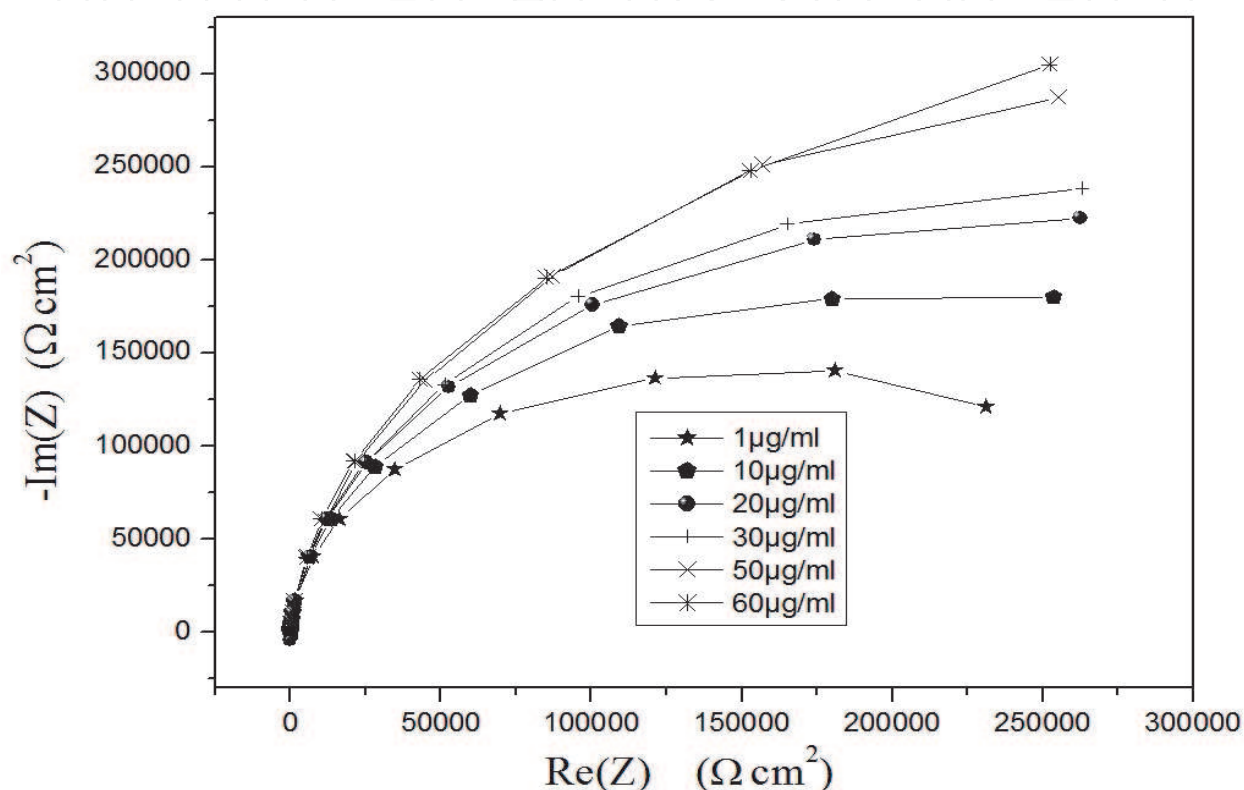


Fig. 2. Impedance spectra of the functionalized gold electrode after the immobilisation of different antibody concentration

The impedance spectra can be fitted with computer simulated program using the electric circuit shown in figure 3. This equivalent circuit includes the ohmic resistance of the electrolyte solution R_0 , the constant phase element Z_{CPE} and electron transfer resistance R_1 . An excellent fitting between the simulated and experimental spectra was obtained for each antibody concentration. Figure4 shows the variation of the impedance versus the antibody concentration. We can see that the surface saturation can be obtained with 60 μg/ml antibody concentration. For specific and non specific antigen detection, we will use this antibody concentration

3.1.1 Virus detection

Figure 5 show the impedance spectra of the functionalized gold electrode recorded at 0 V in PBS buffer at pH=7.2 in the range of 50 mHz to 100 KHz before and after addition of different H₇N₁ antigen concentration.

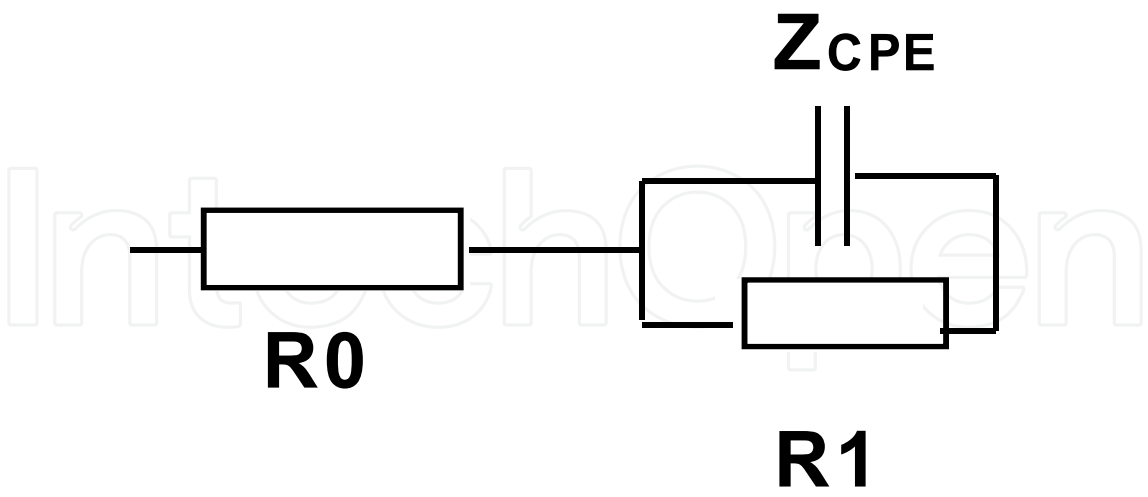


Fig. 3. Electric model

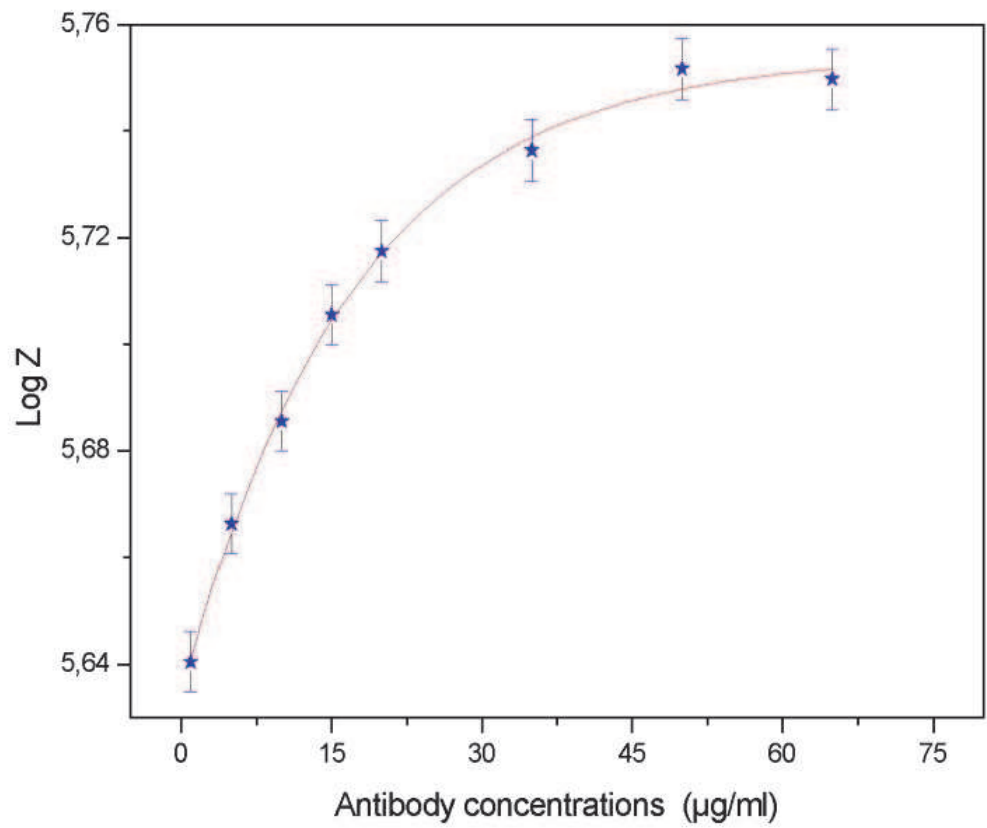


Fig. 4. Impedance spectra of the functionalized gold electrode after the immobilisation of different antibody concentration

The interface can be modeled with the electric model shown in figure3. An excellent fitting between the simulated and experimental spectra was obtained.

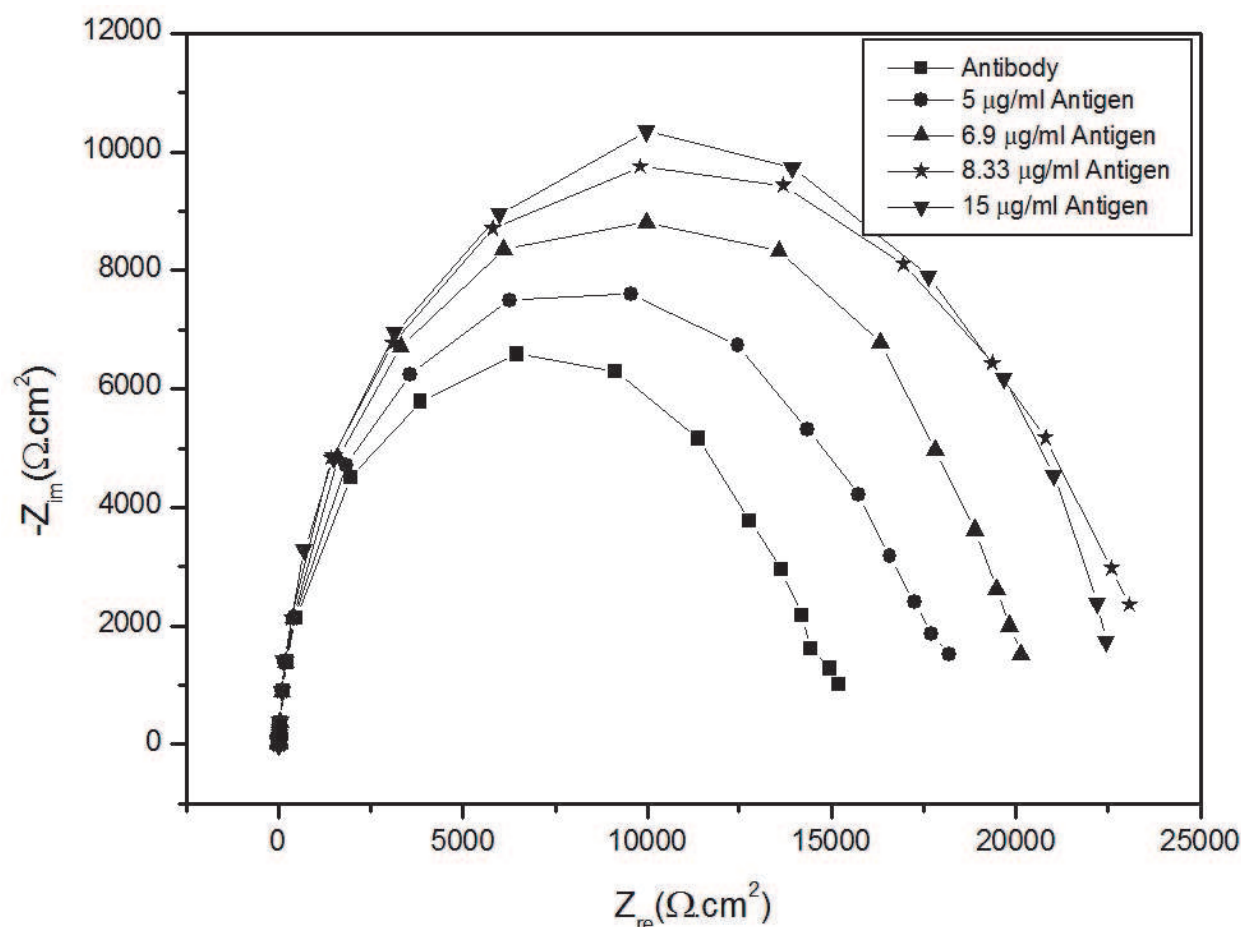


Fig. 5. Impedance spectra of the functionalized gold electrode before and after addition of different H₇N₁ antigen concentration.

The charge transfer resistance increases and reaches a new saturation value that can be determined with the fitting program. This increase could be attributed to a rearrangement in the structure of the antibody and a variation of the dielectric constant. The lowest detection limit that induces a signal variation is equal to 5 µg/ml. This value was lower than the limit detection obtained with ELISA technique.

3.1.2 Calibration and selectivity

In order to obtain the calibration data set, the values of $\log Z/Z_0$ versus the antigen H₇N₁ concentration were plotted in figure 6, where Z is the value of the impedance resistance after antigen binding to antibody, Z_0 is the value of impedance as antibody immobilized on the electrode.

As we can be see in the figure6, the plot is linear and saturate at the higher concentration. To confirm that the above-observed impedance changes generated from the result of specific antibody-antigen interaction, the sensor was exposed to the solution of Newcastle antigen that are expected to bind non-specifically. Figure 6 shows the variation of the impedance

versus the non-specific antigen concentration. As we can see, the sensor was not subjected to the non-specific binding and applicable to the selective determination of H₇N₁.

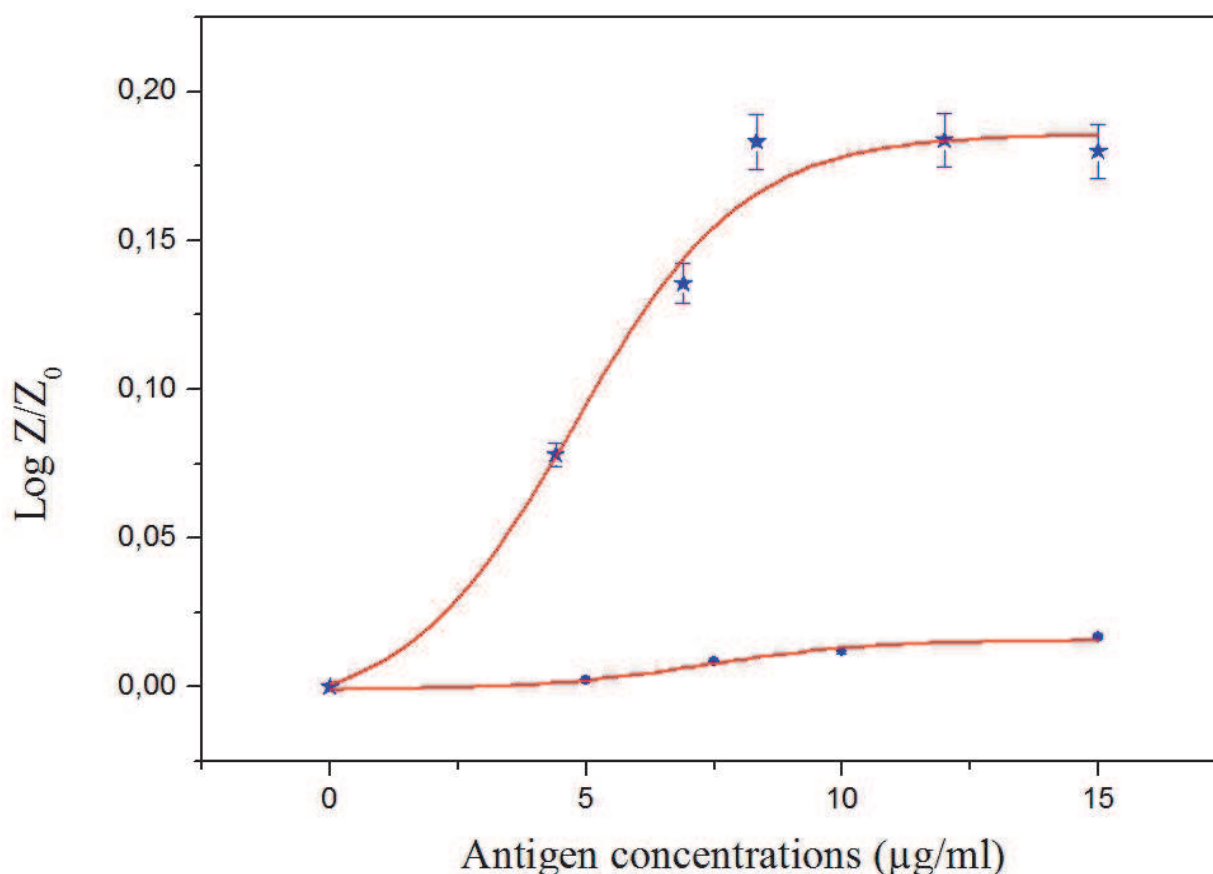


Fig. 6. Calibration curves and selectivity of the developed biosensor.

3.2 Rabbits virus biosensor

We start to characterise the insulating properties of the thiol monolayer on gold surface. The Nyquist diagram of bare gold (fig.7) presents a half-circle, characteristic of a resistance in parallel with a capacity and a linear part which appears at low frequencies and which is assigned to diffusion phenomenon [17]. However, after acid thiol treatment, the diameter of the half-circle of Nyquist diagram increases clearly and the Warburg impedance was not observed. This shows the high insulating properties of the acid thiol (M et al., 2008).

After, impedance measurements were performed after gold surface activation with EDC/NHS, antibody immobilization and BSA blocking step. After each step, acquisitions of impedance data in PBS were carried out over 5 decades of frequency. Figure 8 presents the Nyquist diagram for the various steps of the biosensor development: SAM layer, antibody layer, blocking with BSA and antigen injection.

We observe that each layer deposition on the gold surface generates an impedance increase. This increase is due to the change of the electric properties of the gold/electrolyte interface.

3.2.1 Calibration and selectivity

For rabbits detection, Figure 9 presents the calibration of the developed biosensors for specific and non-specific detection. It shows a dynamic range between 0.1 µg/ml and 4

$\mu\text{g/ml}$ and a saturation reached at $4 \mu\text{g/ml}$. This behaviour can be explained: when the antigen concentration increases in the electrochemical cell, the number of immobilized antibodies, but not complexed, decreases and reaches zero when concentration of antigen is higher than $4 \mu\text{g/ml}$. The limit detection of this sensor is about $0.5 \mu\text{g/ml}$. This limit detection is better than the limit detection obtained with the others traditional methods for clinical use. In order to prove sensor selectivity, the immunosensor was exposed to a solution containing the Newcastle antigen viruses.

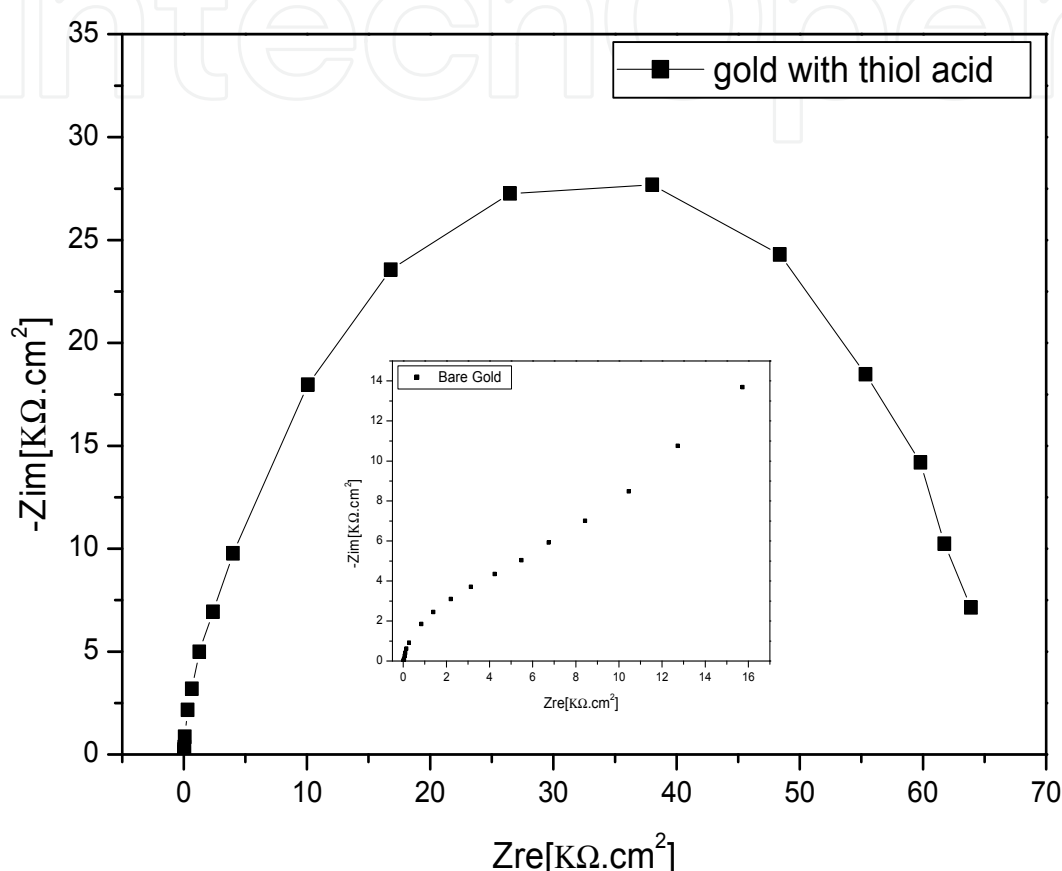


Fig. 7. Nyquist plot for bare gold (small curve) and gold with thiol acid (big curve) in PBS solution with 1 mM redox couple

As shown in figure 9, there is a little variation of impedance after no-specific antigen addition. This little non specific variation can be explained by the use of polyclonal antibodies. In order to avoid non specificity, the use of monoclonal immunoglobulins G (IgGs) is necessary.

4. Conclusion

In this study, we reported the development of biosensor for rabies and for H_7N_1 antigen detection. The affinity interaction of the antibody with specific antigen can be measured with detection limit of 0.5 and $5 \mu\text{g/ml}$ respectively. The impedance spectroscopy technique is a higher sensitive technique which can be used to measure the high insulating properties of biomembranes. The different steps of biosensor conception were characterized by

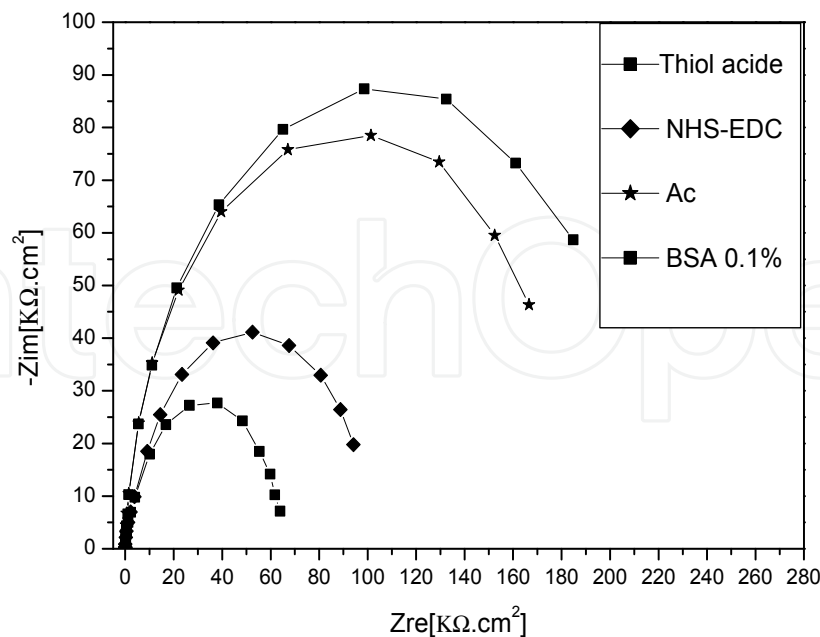


Fig. 8. Nyquist plot of the different layers of the rabies biosensors

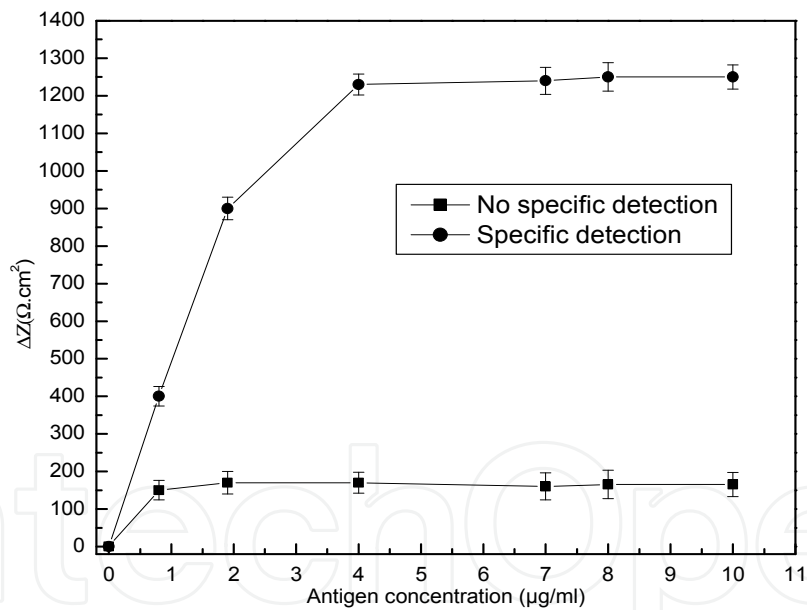


Fig. 9. Selectivity of the developed biosensor.

electrochemical impedance spectroscopy. The sensitivity of miniaturized biosensor prototype will be improved by using interdigitated gold microelectrodes with microfluidic cell for industrial development and clinical use.

5. Acknowledgements

The authors thank the NATO through collaborative Linkage Grant CBP.MD. CLG 982802. and the Alexander Von Humboldt Stiftung (Germany) for the material donation.

6. References

- [1] S, E. Sloan.; C, Hanlon.; W. Weldon.; M, Niezgoda.; J, Blanton. (2007). Identification and characterization of a human monoclonal antibody that potently neutralizes a broad panel of rabies virus isolates. *Vaccine*, Vol.25, pp. 2800-2810.
- [2] L, Martinez.; Global infectious disease surveillance.(2000). *International Journal Infections Diseases* ;Vol. 4, N0. 222, pp. 10-28.
- [3] FX, Meslin.; DB, Fishbein. (1994). Rationale and prospects for rabies elimination in developing countries. *Current Trop Microbiology Immunology*, Vol.187, pp. 1-26.
- [4] World Health Organization. (2002). Rabies vaccines Weekly epidemiological record. Vol. 14, N0. 77, pp. 109-11.
- [5] N, Kamolvarin.; T. Tirawatnpong.; R, Rattanasiwamoke.; S, Tirawatnpong.; T, Panpanich.; and T. Hemachudha. (1993). Diagnosis of rabies by polymerase chain reaction with nested primers. *Journal of Infections Diseases*, Vol. 167, pp.207-210.
- [6] Crepin, P.; L. Audry.; Y. Rotivel.; A. Gacoin.; C. Caroff.; and H. Bourhy. (1998). Intravital diagnosis of human rabies by PCR using saliva and cerebrospinal fluid. *Journal Clinical Microbiology*. Vol, 36, pp. 1117-1121.
- [7] Perrin, P.; and P. Sureau. (1987). A collaborative study of an experimental kit for rapid rabies enzyme immunodiagnosis (RREID). *Bull World Health Organization*.pp.489-493.
- [8] A, Ermine.; N, Tordo.; and H, Tsiang. (1998). Rapid diagnosis of rabies infection by means of a dot hybridization assay. *Molecular Cell Probes*, Vol.2, pp. 75-82.
- [9] G, A.Rand.; J, Ye.; C.W, Brown.; S.V, Letcher. (2002). Optical biosensors for food pathogen detection. *Food Technology*, Vol. 56 , pp.32-37.
- [10] D, Ivnitiski.; I.A, Hamid.; P, Atanasov.; E, Wilkins. (1999). Biosensors for detection of pathogenic bacteria. *Biosensors and Bioelectronics*, Vol. 14 , pp. 599-624.
- [11] J, Homola.; S.S, Yee. ; G, Gauglitz. (1999). Surface plasmon resonance sensors. *Sensors and Actuators B*, Vol. 54 , pp. 3-15.
- [12] A, Tlili.; S, Hleli.; A, Abdelghani.; M.A, Maaref . (2004). Electrical Characterization of a Thiol SAM on Gold as a First Step of the Fabrication of an Immunosensors based on a Quartz Crystal Microbalance. *Sensors*, Vol.4, pp. 104-114.
- [13] S, Hleli.; C, Martelet.; A, Abdelghani.; N, Jaffrezic-Renault. (2006). Atrazine analysis using impedimetric immunosensors based on mixed biotinylated self-assembled monolayer. *Sensors and Actuators B*, Vol.113 , pp. 711-717.
- [14] A, Abdelghani.; K, Cherif.; M, Maaref. (2006). Impedance Spectroscopy on Xerogel Layer for Chemical Sensing. *Materials Science and Engineering C*, Vol. 26, pp. 542 - 545.
- [15] A, Tlili.; A, Abdelghani.; S, Ameur.; N, Jaffrezic-Renault. (2006). Impedance spectroscopy and affinity measurement of specific antibody-antigen interaction. *Materials Science and Engineering C*, Vol. 26, pp. 546 - 550.
- [16] M, Hnaïen.; S, Hleli.; M, Diouani.; I, Hafaid.; W, Hassen.; N, Jaffrezic- Renault.; A, Abdelghani. (2008). Immobilisation of Specific Antibody on SAM Functionalized Gold Electrode for Rabies Virus Detection by Electrochemical Impedance Spectroscopy. *Biochemical Engineering Journal*, Vol. 39, N0. 3, pp. 443-449.
- [17] M, .Diouani.; S, Hleli.; I, Hafaid.; A, Snousi.; A,Ghram.; A,Abdelghani. (2008). Immobilisation of Specific Antibody on Fonctionnalisés Gold Microelectrode for Avian Influenza Virus H7N1 Detection. *Materials Science and Engineering C*, Vol. 28, N0. 5-6 , pp. 580-583.



Biosensors for Health, Environment and Biosecurity

Edited by Prof. Pier Andrea Serra

ISBN 978-953-307-443-6

Hard cover, 540 pages

Publisher InTech

Published online 19, July, 2011

Published in print edition July, 2011

A biosensor is a detecting device that combines a transducer with a biologically sensitive and selective component. Biosensors can measure compounds present in the environment, chemical processes, food and human body at low cost if compared with traditional analytical techniques. This book covers a wide range of aspects and issues related to biosensor technology, bringing together researchers from 16 different countries. The book consists of 24 chapters written by 76 authors and divided in three sections: Biosensors Technology and Materials, Biosensors for Health and Biosensors for Environment and Biosecurity.

How to reference

In order to correctly reference this scholarly work, feel free to copy and paste the following:

Abdelghani Adnane (2011). Electrochemical Biosensors for Virus Detection, Biosensors for Health, Environment and Biosecurity, Prof. Pier Andrea Serra (Ed.), ISBN: 978-953-307-443-6, InTech, Available from: <http://www.intechopen.com/books/biosensors-for-health-environment-and-biosecurity/electrochemical-biosensors-for-virus-detection>

INTech
open science | open minds

InTech Europe

University Campus STeP Ri
Slavka Krautzeka 83/A
51000 Rijeka, Croatia
Phone: +385 (51) 770 447
Fax: +385 (51) 686 166
www.intechopen.com

InTech China

Unit 405, Office Block, Hotel Equatorial Shanghai
No.65, Yan An Road (West), Shanghai, 200040, China
中国上海市延安西路65号上海国际贵都大饭店办公楼405单元
Phone: +86-21-62489820
Fax: +86-21-62489821

© 2011 The Author(s). Licensee IntechOpen. This chapter is distributed under the terms of the [Creative Commons Attribution-NonCommercial-ShareAlike-3.0 License](https://creativecommons.org/licenses/by-nc-sa/3.0/), which permits use, distribution and reproduction for non-commercial purposes, provided the original is properly cited and derivative works building on this content are distributed under the same license.

IntechOpen

IntechOpen